

Fig. 1

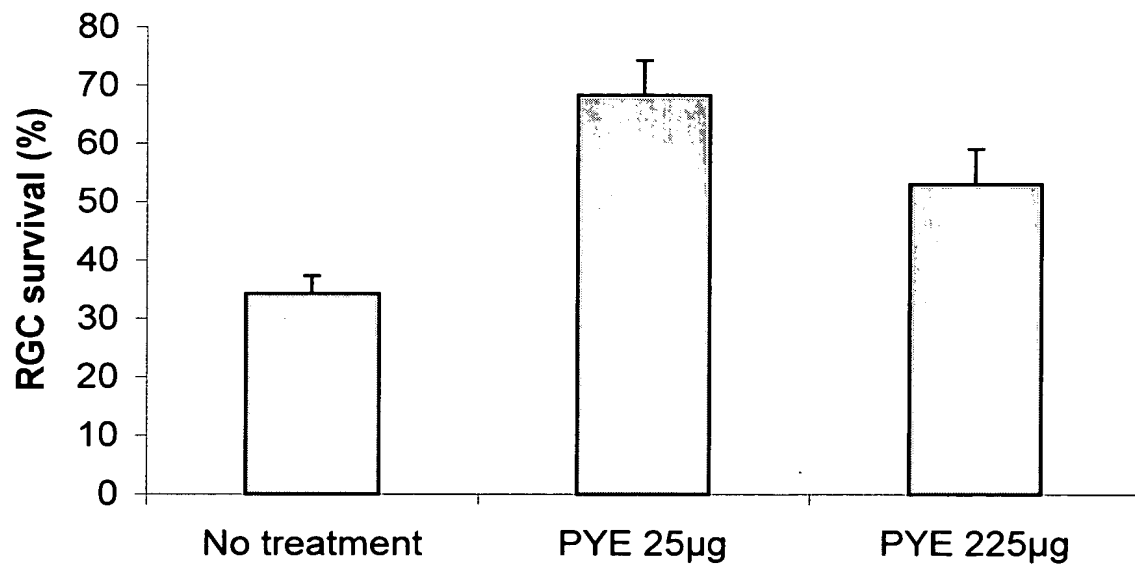


Fig. 2

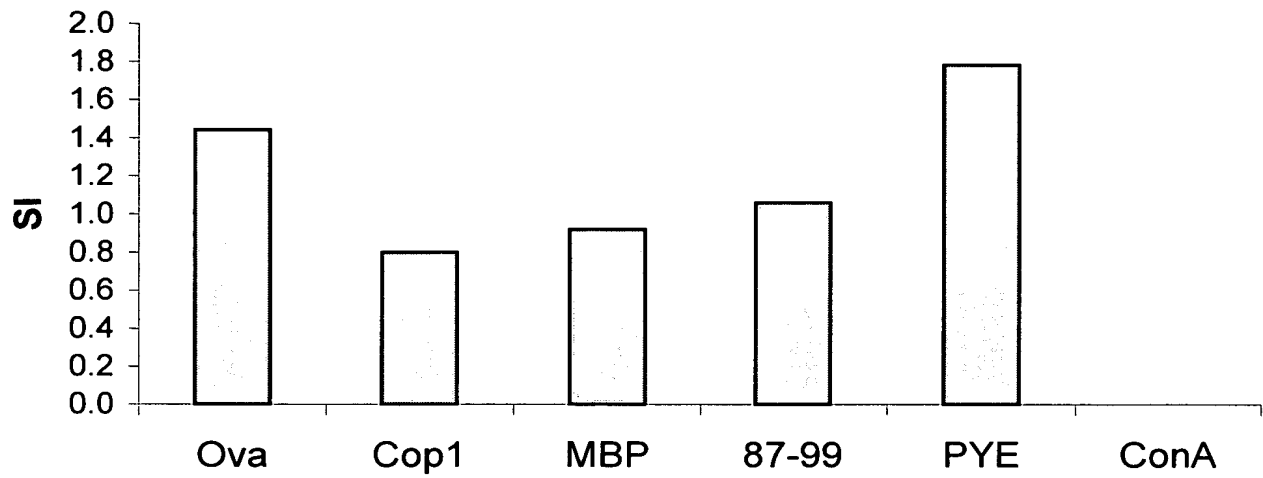


Fig. 3

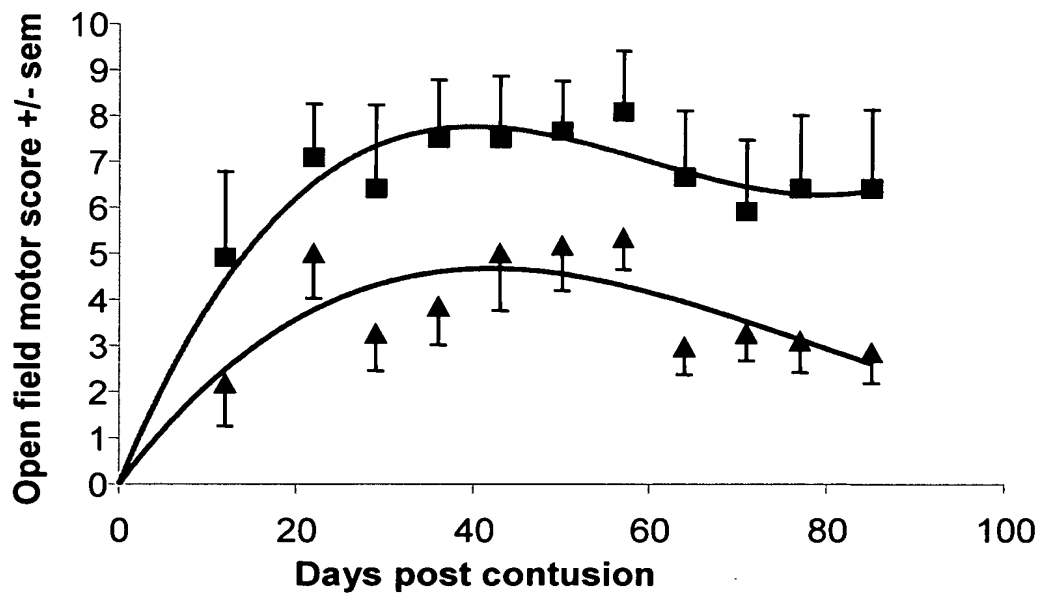


Fig. 4A

3/14

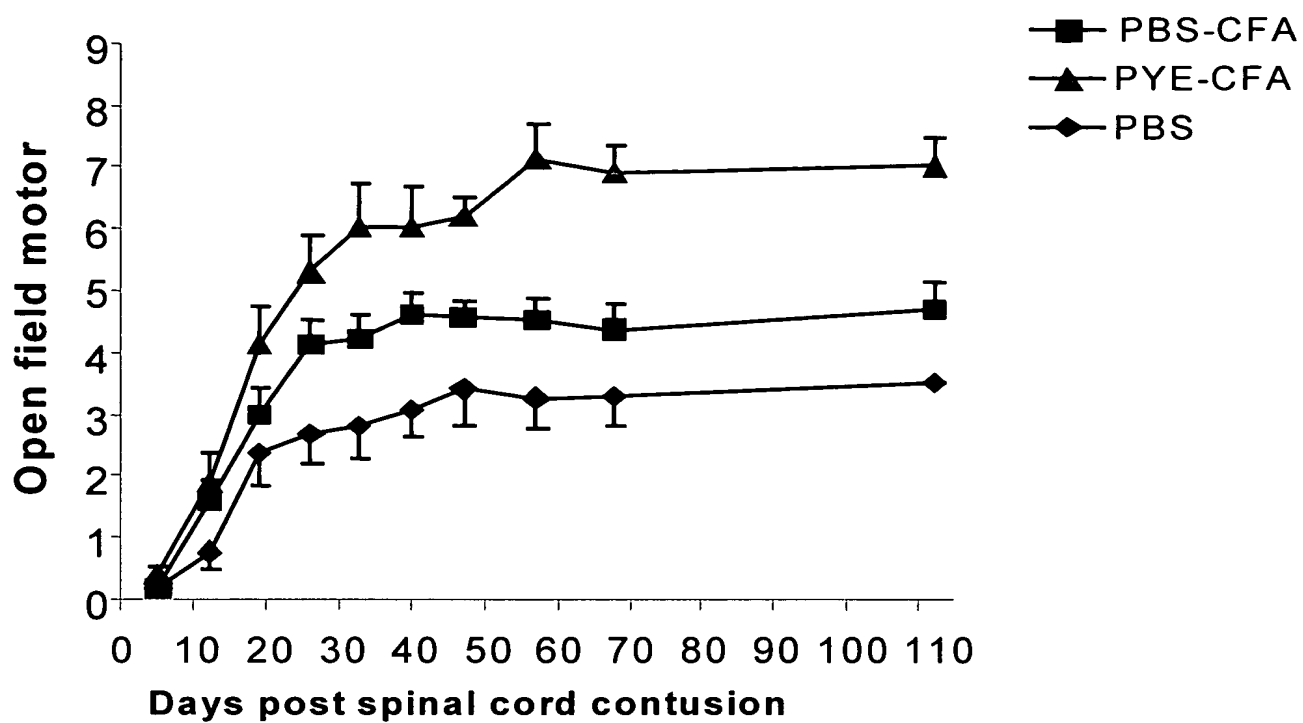


Fig. 4B

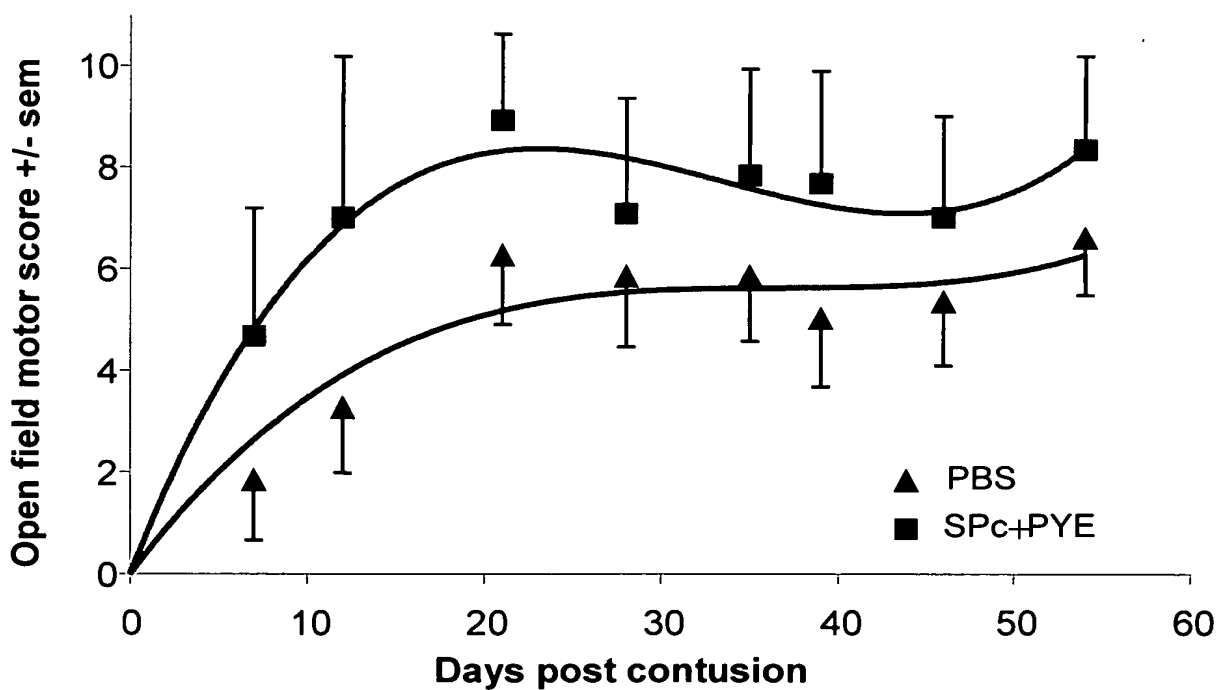


Fig. 5

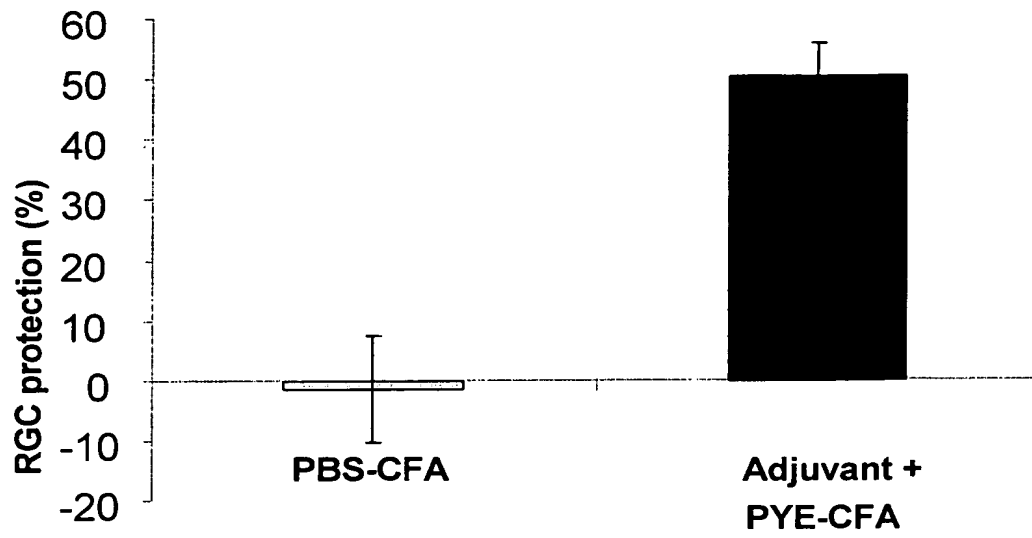


Fig. 6

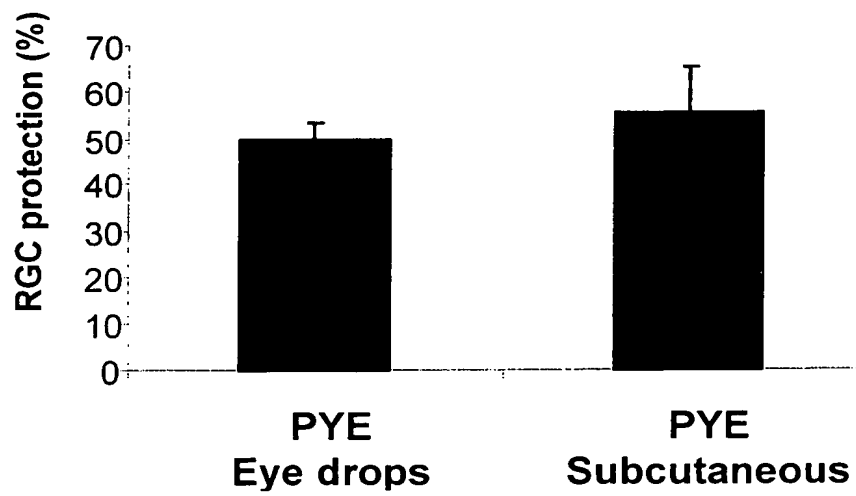


Fig. 7

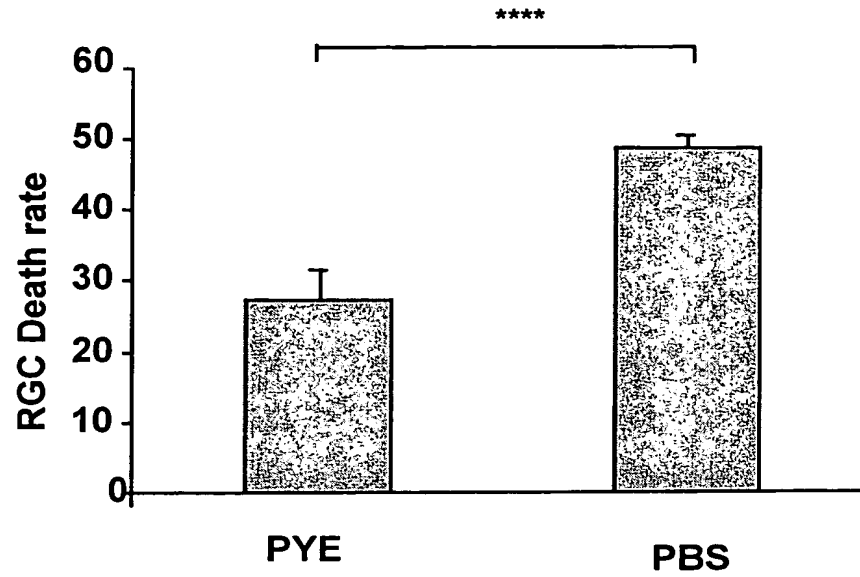


Fig. 8

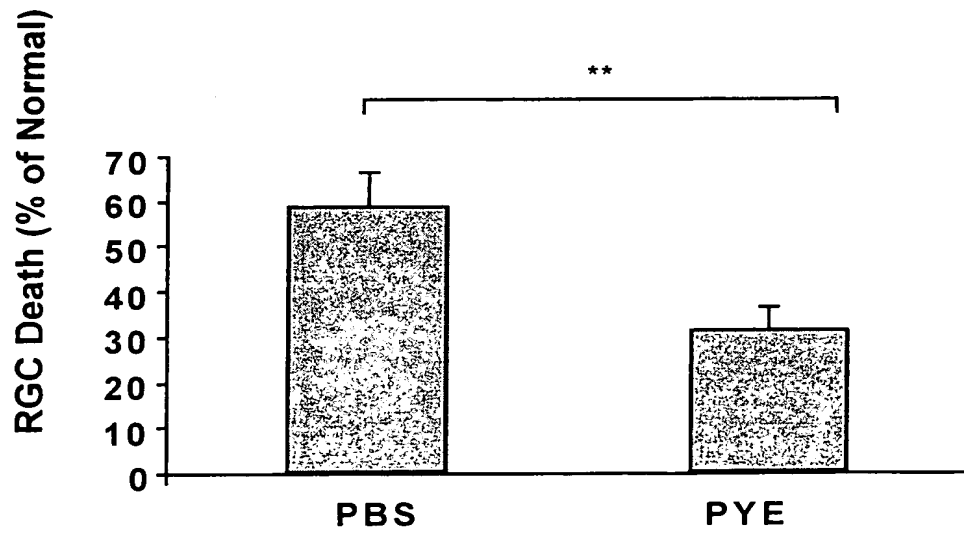


Fig. 9

6/14

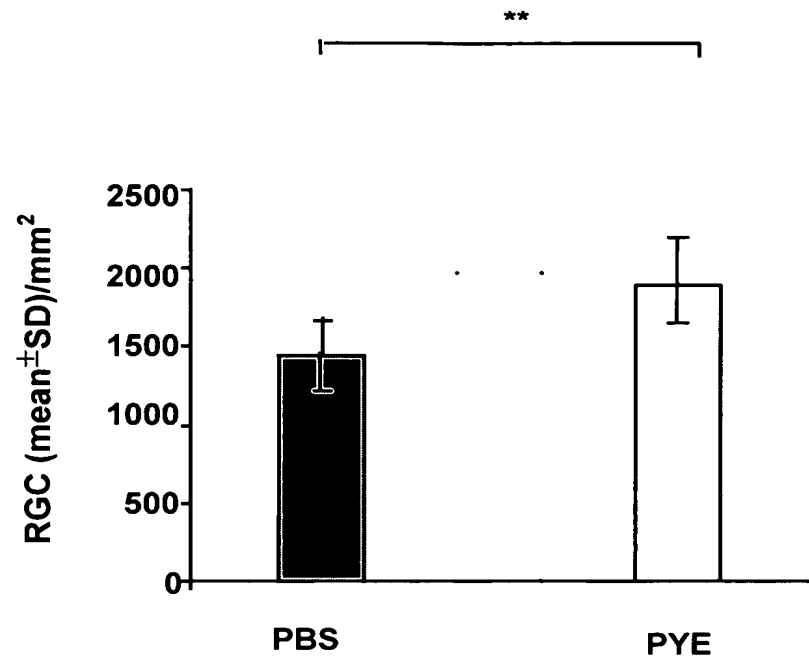


Fig. 10

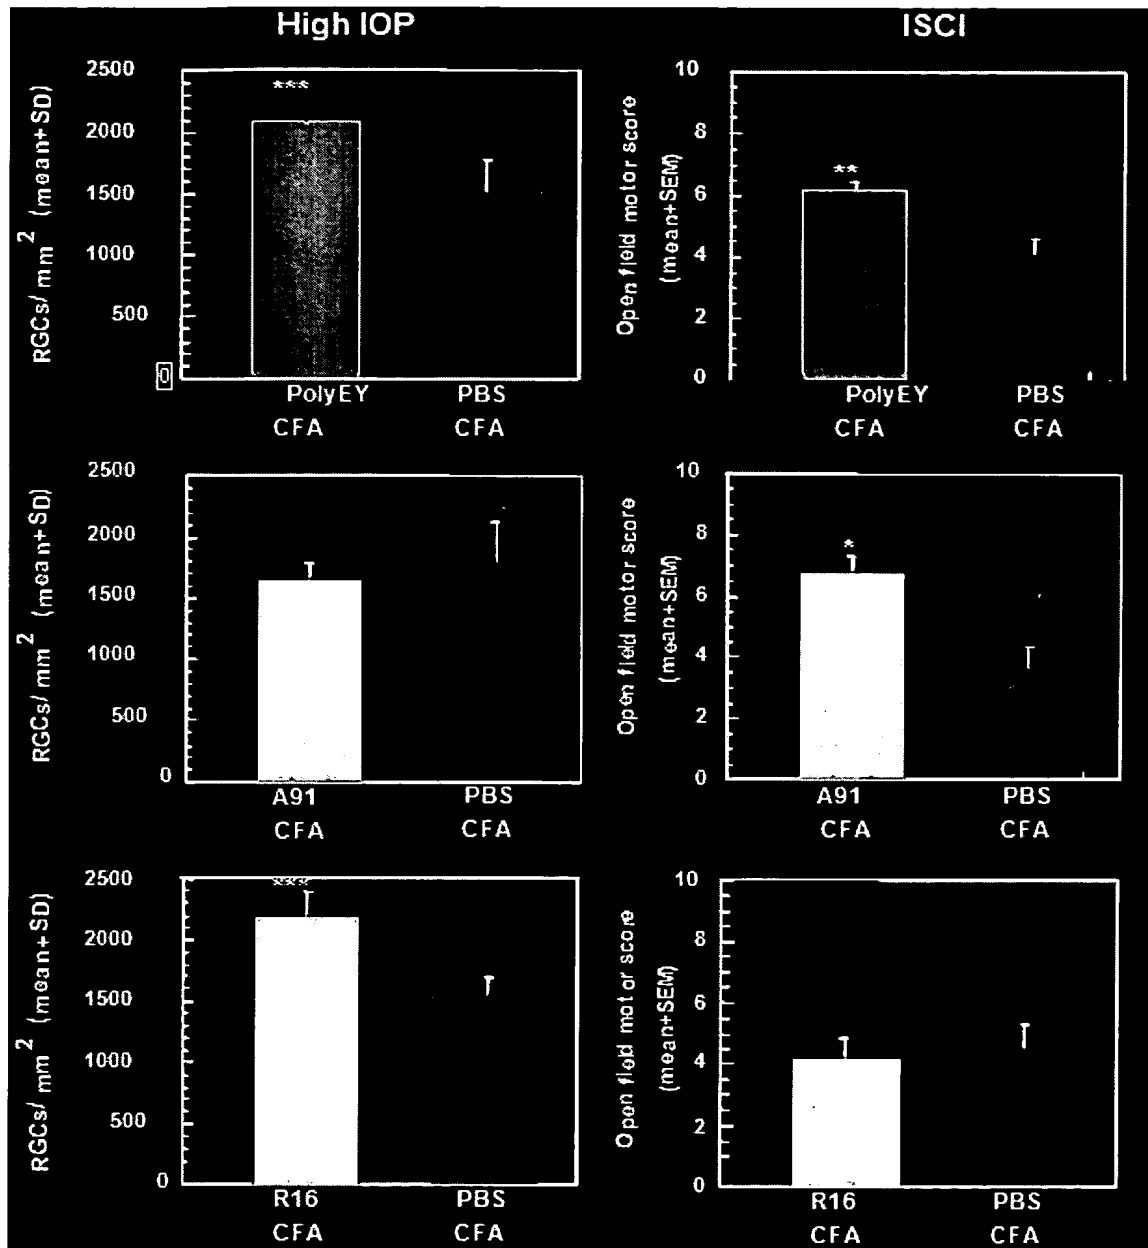


Fig. 11

8/14

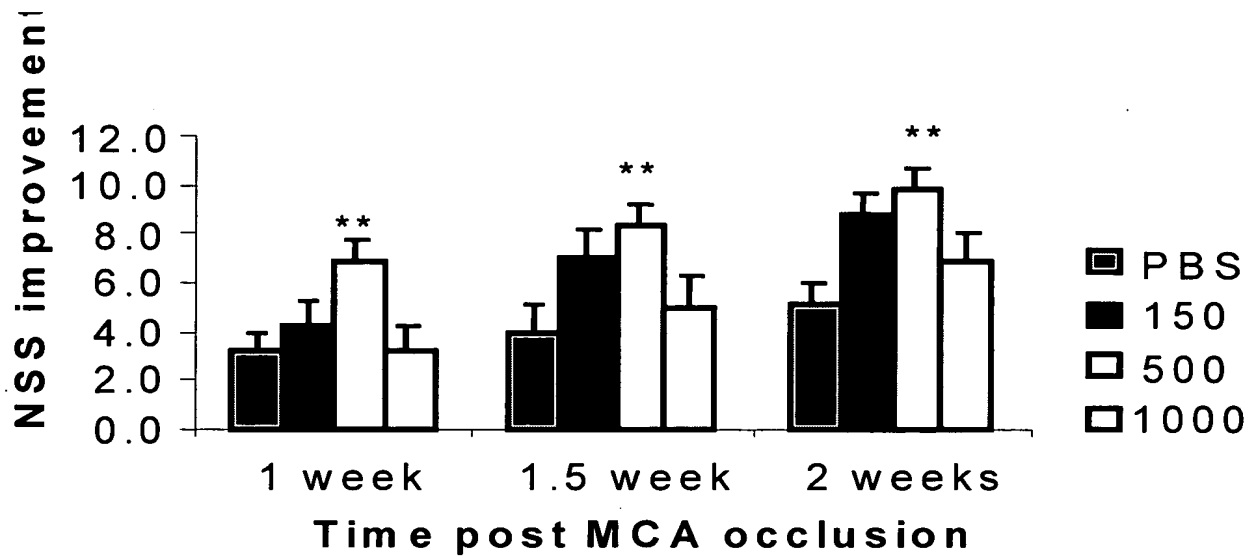


Fig. 12

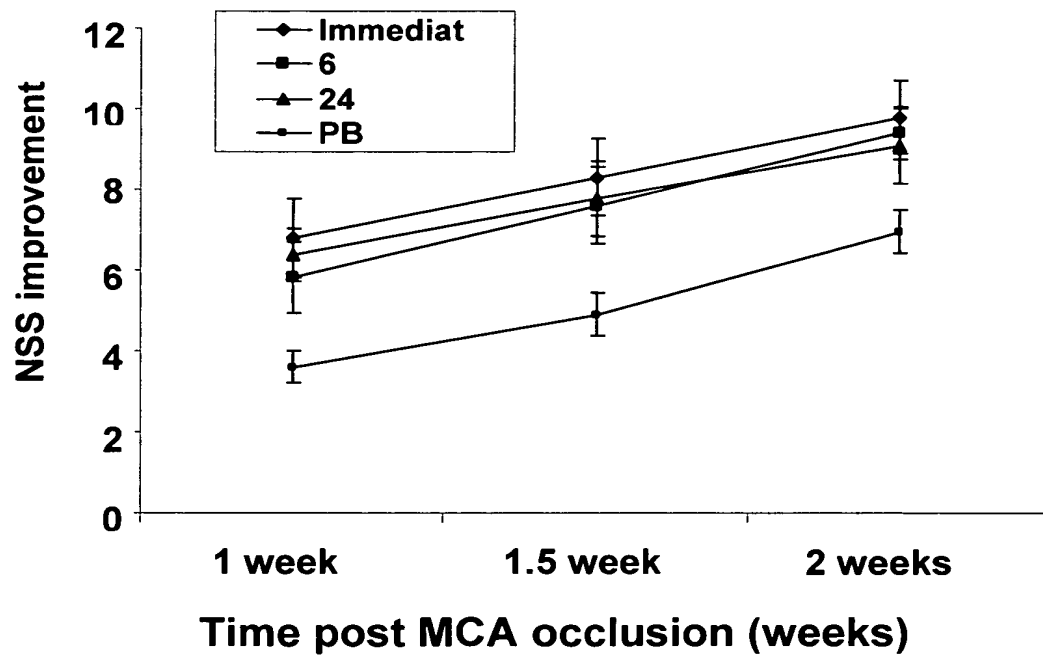


Fig. 13

9/14

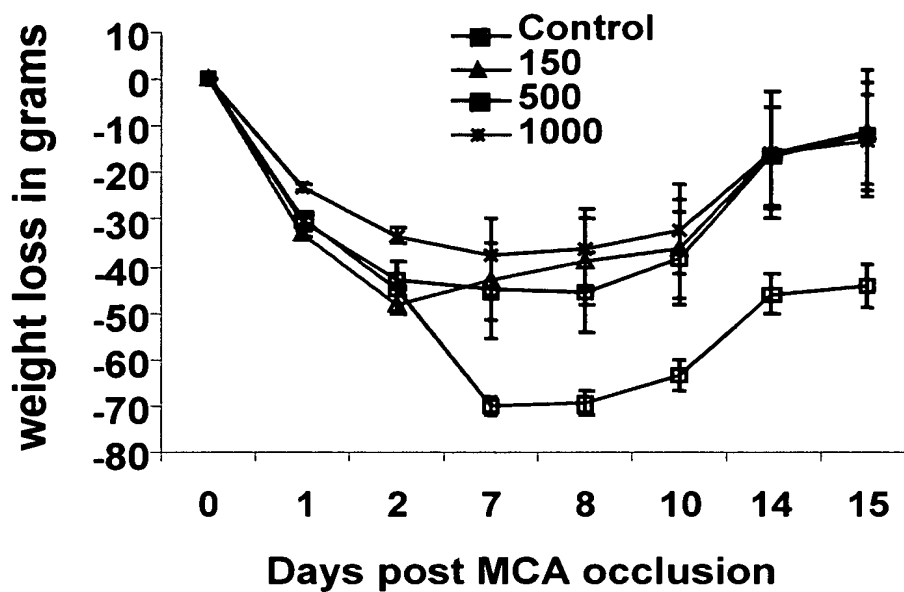


Fig. 14

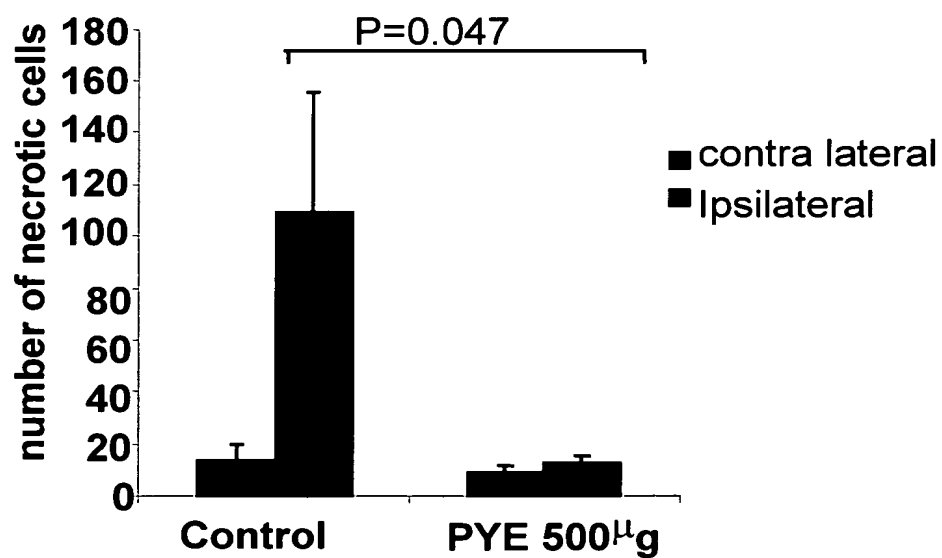


Fig. 15

10/14

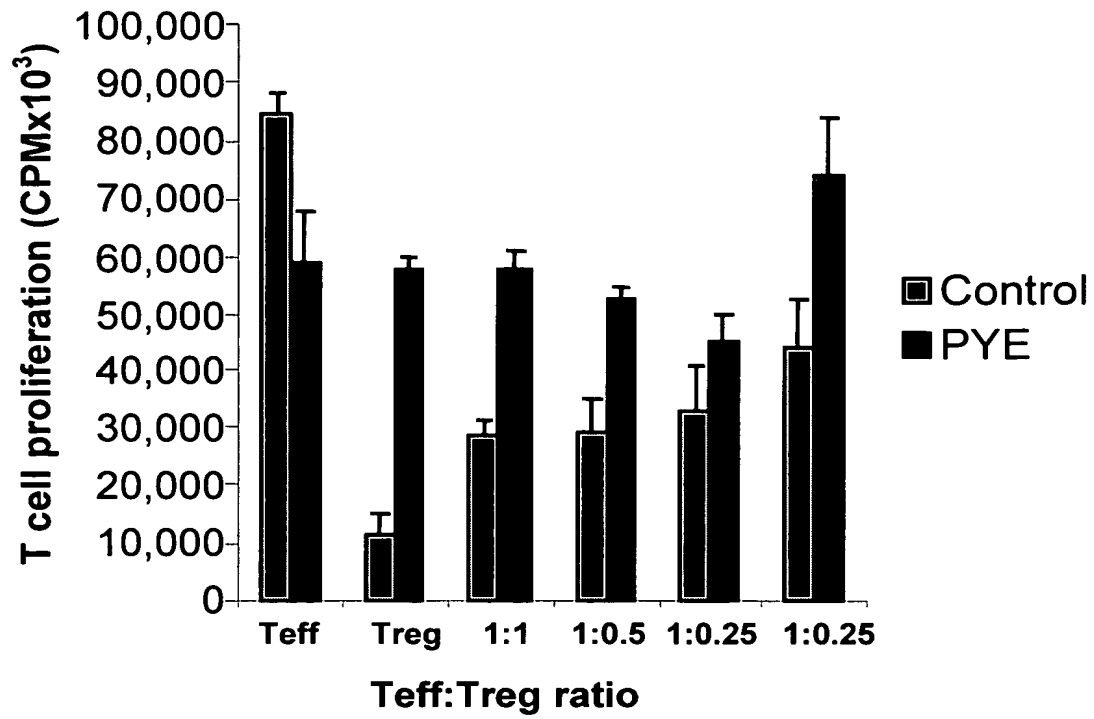


Fig. 16A

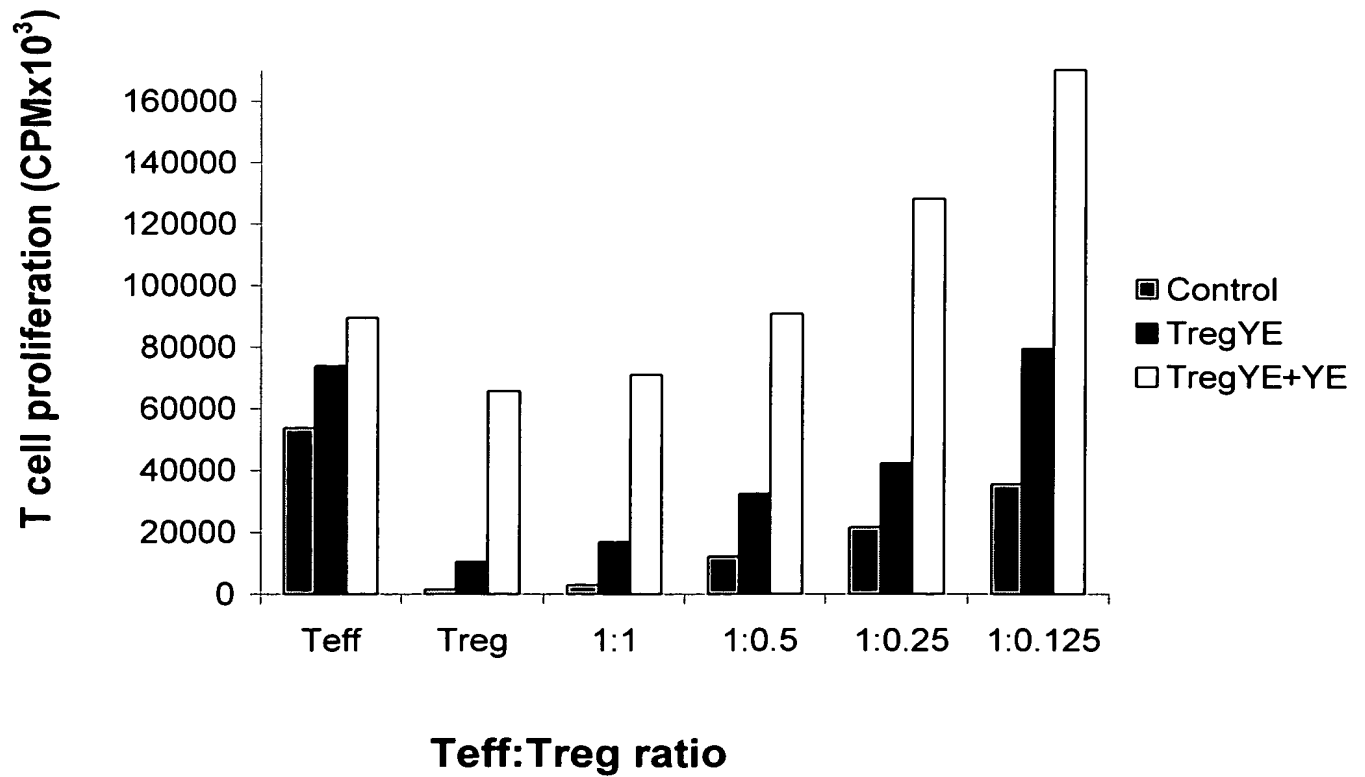


Fig. 16B

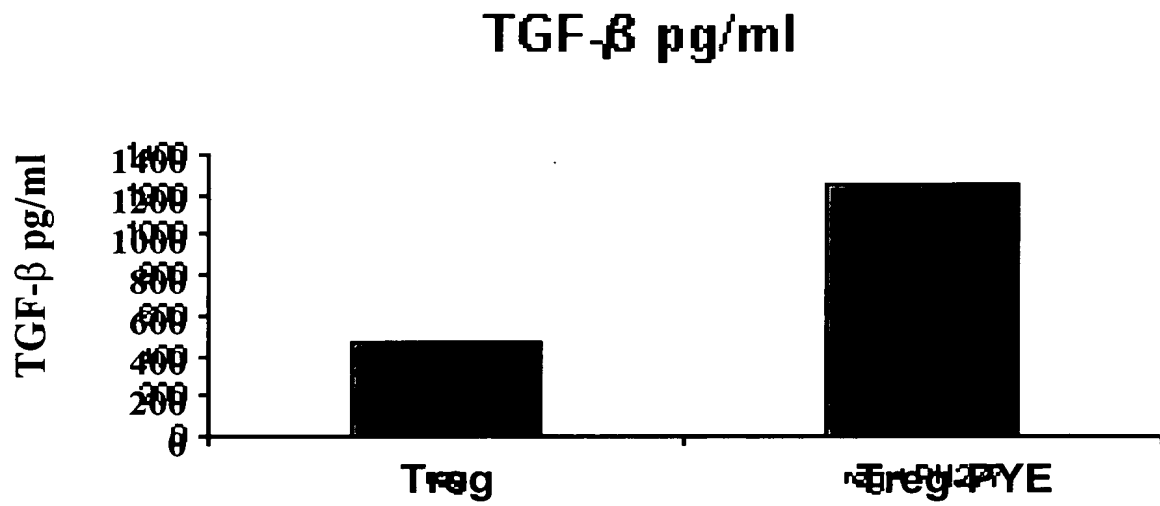
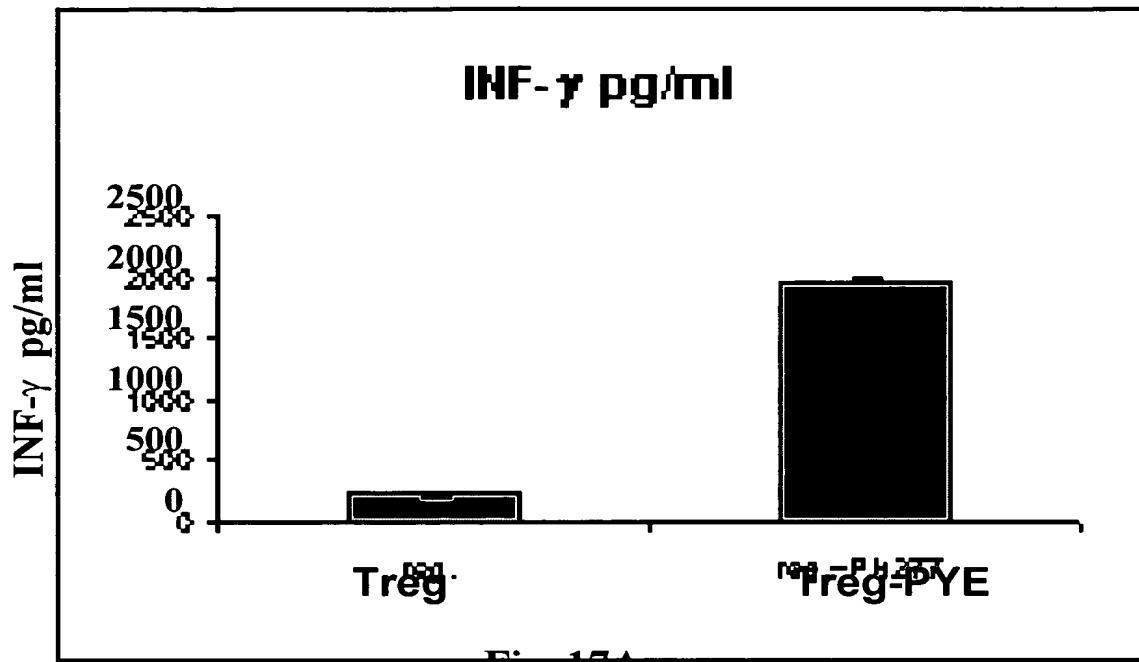


Fig. 17B

12/14

IL-2 pg/ml

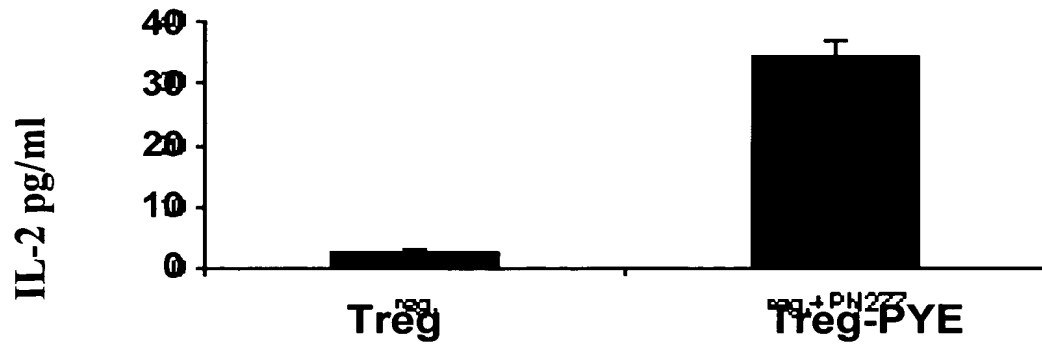


Fig. 17C

IL-10 pg/ml

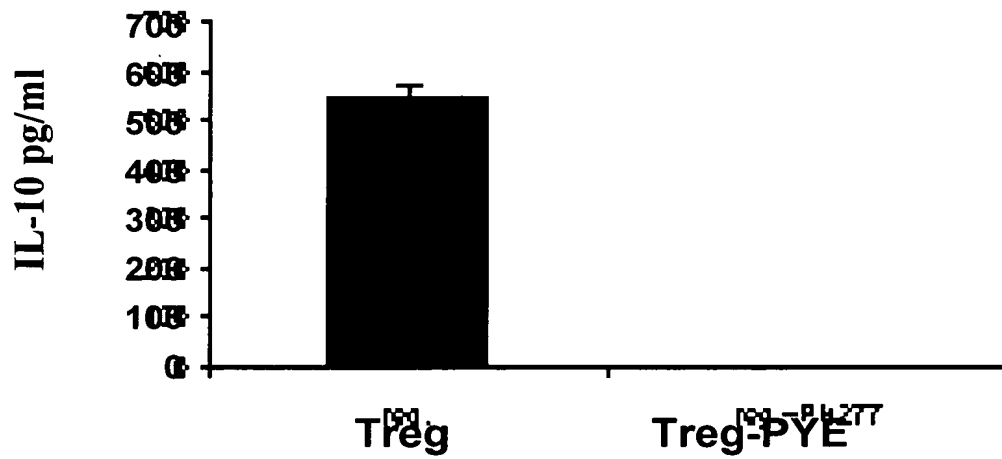




Fig. 17D

13/14

MK-801 + YE DAY 1 -

INPUT 1

MK 801 + PBS

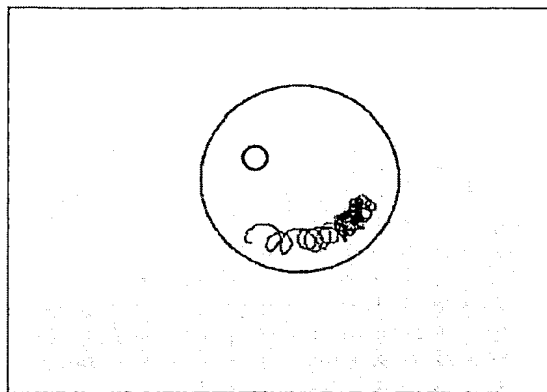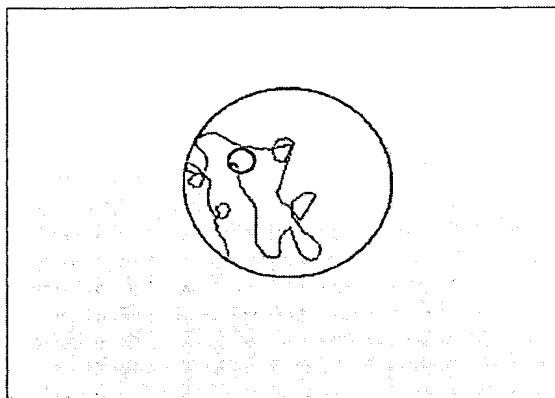

INPUT 4

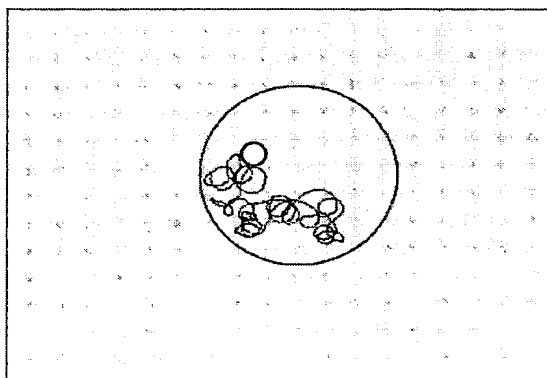
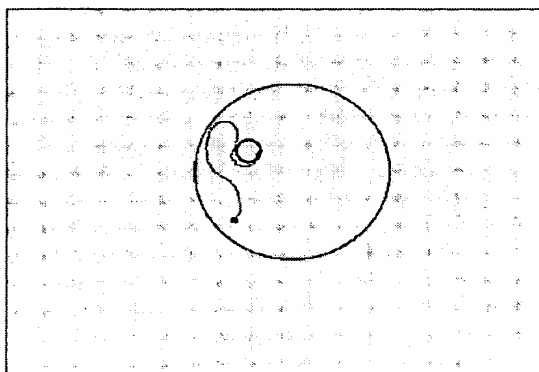


Fig. 18

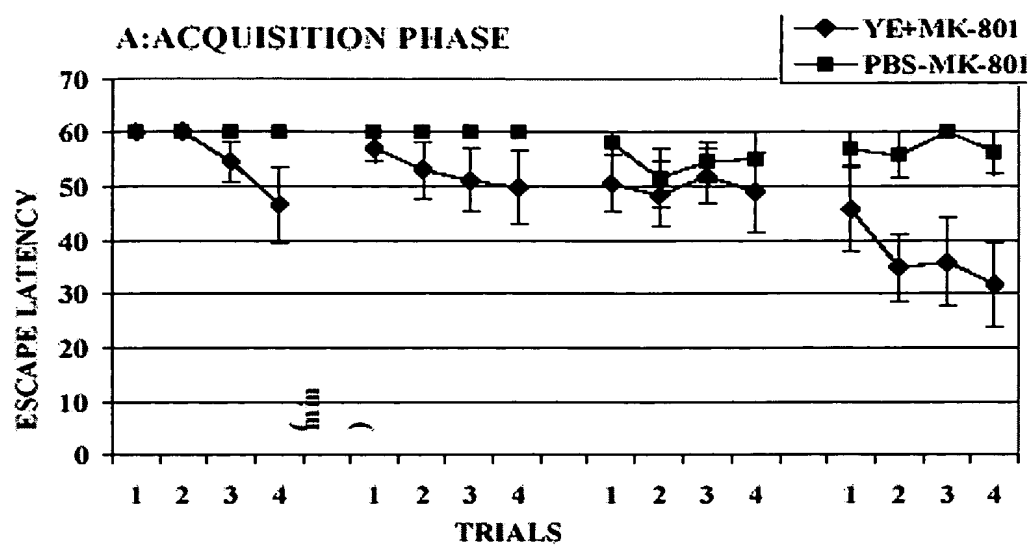


Fig. 19